






EMS® P3D

Order Code 6680654

Satelec® P3-SD

Order Code 6680636

Function Description: Used to level off the surface of endo after the periodontal flap surgery

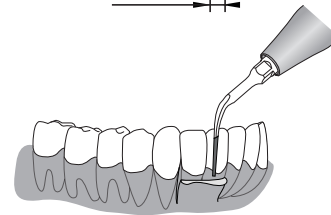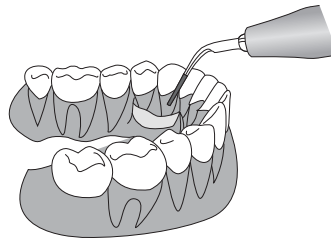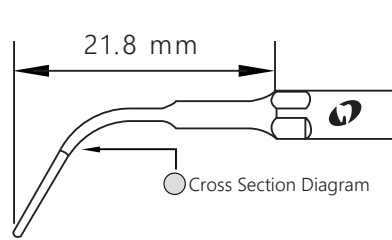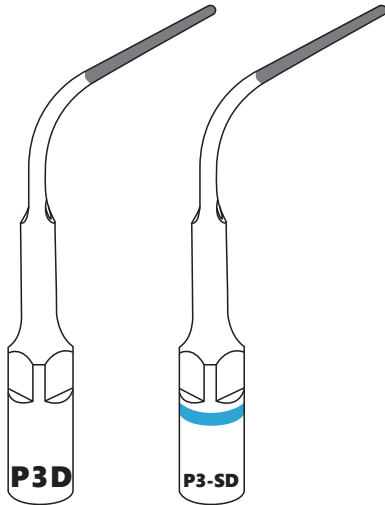

Mode: P  
Power: 1-6



Recommended  
Service Life  
50 Teeth



Water Flow Rate  
mid&high